

RAPID Slit Seal

RAPID Slit Seal Instruction Manual

Thank you for purchasing our RAPID Slit Seal.
Please read this manual carefully before use and
save this manual for your future use.

Please note that product specifications and packings
may change without prior notice.

Announcement for your use with ease.

【Purpose of use】

This product can be used for research purposes only.

【Notes for use】

Handle this product carefully when unpacking from the bag.

Do not process this product in autoclave treatment.

【Storage and disposal of product】


Store at room temperature and in a place not exposed to direct
sunlight. To dispose the product after use, comply with local laws
and ordinances, and process properly according to the regulations
of your facility.

Instructions

*Please wear gloves before use.

1


The film with a red indication is a release liner.

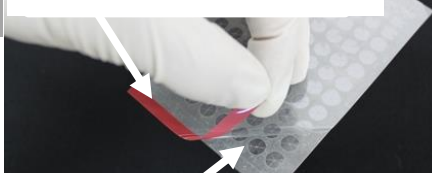

Peel off the release liner to expose the adhesive surface.

Remove the release liner with a red indication and expose the adhesive
surface.

2

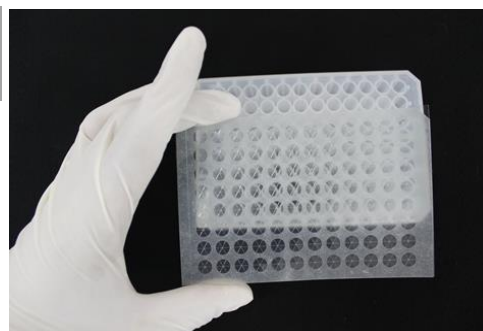

Paste the RAPID Slit Seal on the 96-well plate and make sure
holes of RAPID Slit Seal are correctly positioned on each well
spot.

3



Remove the protective film before sampling or dispensing. If used
without removing the protective film, the needle or the tip can not
puncture the film. If the protective film stays on and is left at 100°C,
the edge of the protective film may be curved.

Manufacturer



BioChromato, Inc.

1-12-19 Honcho, Fujisawa, Kanagawa-ken 251-0053 JAPAN

TEL : +81-466-23-8382 FAX : +81-466-23-8279

E-mail : oversea@bier.co.jp

Website: <https://biochromato.com/>

Catalog Code	RSS-S96-80122	R80.120.00
	R80.120.10	R80.120.50
Product name	RAPID Slit Seal	
Bonding method	Pressure sensitive adhesive	
Materials	PET, Silicone	
Operating temperature limit	-80°C~100°C *	
Size	W 80 mm × L 122 mm	
Quantity	RSS-S96-80122 R80.120.00 : 100 sheets/Box	
	R80.120.10 : 10 sheets/Box	
	R80.120.50 : 10 sheets/Box × 5 boxes	

* The upper limit of the operating temperature is specified as 100 ° C, and this is clarified by the evaluation test carried at
100 ° C for 30 minutes.